

MICROMAC COD-Cr

ON LINE ANALYZER FOR WATER AND WASTEWATER
COD-Cr MONITORING IN WATER

MICROMAC COD is a microprocessor controlled On Line analyzer specifically designed for automatic COD Potassium Dichromate method monitoring on several types of waters matrix.

✓ **ROBUST AND RELIABLE**

Designed for industrial and Environmental On Line applications ensures the highest level of robustness in the electronics, mechanics and hydraulics components. Complete separation between electronics and hydraulics plus a simple and robust LFA * hydraulics allows easy maintenance and long terms reliable operations.

✓ **AUTOMATIC CALIBRATION**

When the Calibration Time interval expires the analyzer performs a Calibration Cycle, storing and checking the new calibrant O. D. If new O.D. exceeds selected limits, an alarm contacts is closed.

✓ **EASY TO INSTALL**

The analyzer is delivered after a long and successful series of factory tests ready for installation and setup; it is provided with complete set of spares for start up. To start monitoring is enough to connect reagents, sample line, waste line and power supply.

✓ **MEASURING INTERVAL**

User selectable; between two measurements the analyzer remains in stand by mode, without reagents consumption.


✓ **FEATURES AND BENEFITS**

- Fully automatic operation
- Long autonomy; low maintenance, low operating cost
- Low reagents consumption; short preparation time; low disposable costs
- Easy operation; plug in analyzer, no special training is required
- Electronics and hydraulics completely separated
- Serial interface for local o remote PC connection (optional)

COD-Cr measuring principle and hydraulic diagram

The sample after proper filtration is pumped inside the digestion unit, where Mercury Sulfate, Sulfuric Acid and Potassium Dichromate are injected. After mixing the sample is heated at 170° C, typically 5-15 minutes. When digestion time expires the reaction product is cooled then the sample measured by a detector integrated in the digestion unit

The measured absorbance is used for the calculation of the sample concentration against the stored calibration factor.

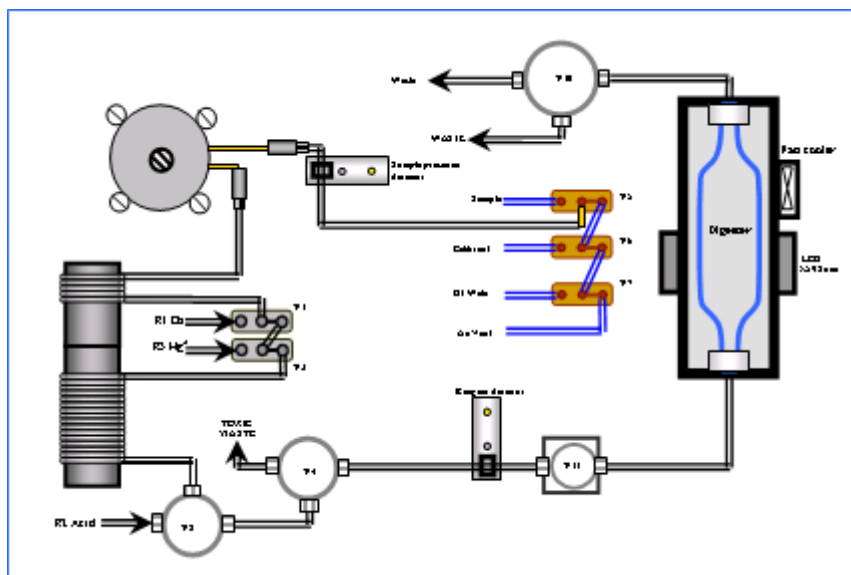

Technical Specifications

MEASURING PRINCIPLE: Colorimetric, after digestion with potassium dichromate and sulfuric acid

COLORIMETER: dual beam, silicon detector

MEASUREMENT TYPE: cyclic

MEASURING INTERVAL: programmable

MEASURING TIME: 25-35 minutes (depending on the measurement range & digestion time)

MEASURING RANGE: 0-50/100/200/300/500/1000/2000 ppm COD, other ranges available on request

DETECTION LIMIT: typical 5% of the full scale, calculated as for EPA p. 136 appendix B

REPEATABILITY: better than 5% ; SD% of 7 replicates at 50% of the full scale

ACCURACY: better than 5% 7 replicates at 20% of the full scale

OUTPUT SIGNAL: 4-20 mA

INPUT SIGNALS: n. 1 Analysis, n. 1 calibration; digital contacts

ALARMS: n. 1 High Limit, n. 1 General, n. 1 Calibration; potential free contacts

SAMPLE AND WASTE DELIVERY: pressure free; **SAMPLE TEMPERATURE:** 10°C - 30 °C

REAGENTS REPLACEMENT: 4/5 weeks

PROTECTION: IP55

HARDWARE: PC104 industrial standard, Integrated keyboard and graphics display, RS232 option

POWER SUPPLY: 12 VDC analyzer + 24 V AC digester external power supply included; 4W Standby; 90 W (mean) analysis

WEIGHT: 33 Kg without reagents:

DIMENSION: 800x420x280 mm(hxwx d)

Subject to change without notice

**SYSTE A S.p.A.**

HEADQUARTER AND MANUFACTURING FACILITY:

VIA PADUNI, 2A - 03012 ANAGNI (FR) ITALY

TEL: +39 0775-776058 FAX +39 0775-772204

A member of Consorzio NDI

Web Site: <http://www.systea.it> Email: info@systea.it

Document ID: MicC CODCr-09-E DR (20151209)