

MICROMAC COD-Mn

ON LINE ANALYZER FOR COD-Mn MONITORING IN WATER AND SEAWATER



MICROMAC COD-Mn is a microprocessor controlled On Line analyzer specifically designed for automatic COD-Mn monitoring on several types of water matrix, including seawater.

✓ ROBUST AND RELIABLE

Designed for industrial and Environmental On Line applications ensures the highest level of robustness in the electronics, mechanics and hydraulics components. Complete separation between electronics and hydraulics plus a simple and robust LFA * hydraulics allows easy maintenance and long terms reliable operations.

** LFA: Loop Flow Analysis patent pending*

✓ EASY TO INSTALL

The analyzer is delivered after a long and successful series of factory tests ready for installation and setup; it is provided with complete set of spares for start up. To start monitoring is enough to connect reagent, sample line, waste line and power supply.

✓ AUTOMATIC CALIBRATION

When the Calibration Time interval expires the analyzer performs a Calibration Cycle, storing and checking the new calibrant O. D. If new O.D. exceeds selected limits, an alarm contacts is closed.

✓ SAMPLE DILUTION

Sample can be analyzed as it is or after automatic dilution. Automatic dilution is factory adjusted for high range applications.


✓ MEASURING INTERVAL

User selectable; between two measurements the analyzer remains in stand by mode, without reagents consumption.

✓ FEATURES AND BENEFITS

- Fully automatic operation
- Long autonomy; low maintenance, low operating cost
- Low reagents consumption; short preparation time; low disposable costs
- Easy operation; plug in analyzer, no special training is required
- Electronics and hydraulics completely separated
- Serial interface for local o remote PC connection (option)

COD-Mn measuring principle and hydraulic diagram

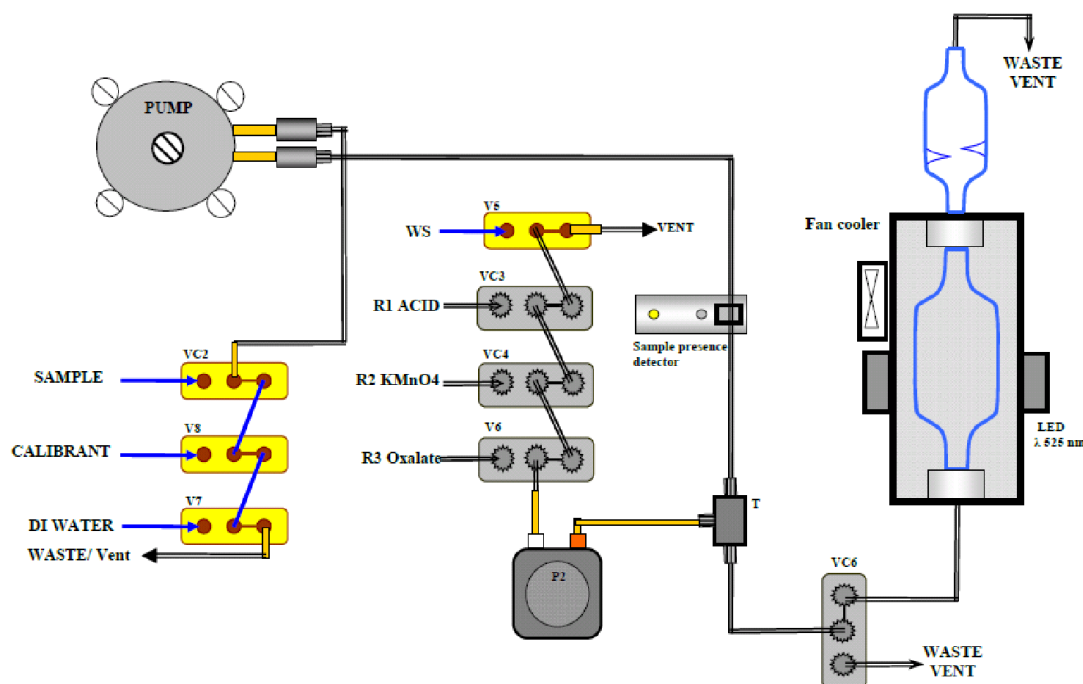

The sample is pumped inside the digestion tube, together diluted sulphuric acid, at about 100°C starts the addition of KMnO_4 , addition volume depends on the analyzer range. After digestion, an excess of oxalate is added to reduce the excess of permanganate; the remaining, oxalate, proportional to the original content of organic, is oxidised by another addition of permanganate; after a proper cooling time the analyzer read the colour directly in the digester: The decrease of the absorbance is measured at 525 nm corresponds to the permanganate consumed by the organic substance

Technical Specifications

MEASURING PRINCIPLE: Colorimetric, after digestion with potassium dichromate and sulfuric acid

COLORIMETER: dual beam, silicon detector

MEASUREMENT TYPE: cyclic; **MEASURING INTERVAL:** programmable;

MEASURING TIME: minimum. 30 minutes

MEASURING RANGE: 0-5/10/20/50/100mg/L O, other ranges available on request

DETECTION LIMIT: 0.1mg/L, calculated as for EPA p. 136 appendix B

REPEATABILITY: better than 2%; **ACCURACY:** +/-5%

ZERO DRIFT: 1% FS; **RANGE DRIFT:** 1% FS; **RESOLUTION:** 0.001

OUTPUT SIGNAL: 4-20 Ma; **INPUT SIGNALS:** n. 1 Analysis, n. 1 calibration; digital contacts

ALARMS: n. 1 High Limit, n. 1 General, n. 1 Calibration; potential free contacts

SAMPLE AND WASTE DELIVERY: pressure free; **SAMPLE TEMPERATURE:** 10°C - 30 °C

REAGENTS CHANGE: 30 days

PROTECTION: IP55

HARDWARE: PC104 industrial standard, Integrated keyboard and graphics display, RS232 option

POWER SUPPLY: 12 & 24 VDC external power supply included; 10W Standby; 40 W (mean) analysis

WEIGHT: 33 Kg without reagents; **DIMENSION:** 800x420x280 mm(hxwx d)

Subject to change without notice



SYSTEA S.p.A.

MAIN OFFICE, PRODUCTION AND SERVICE:

VIA PADUNI, 2A - 03012 ANAGNI (FR) ITALY

TEL: +39 0775-776058 FAX +39 0775-772204

A member of Consorzio NDI

Web Site: <http://www.systea.it> Email: info@systea.it

Document ID: Mic_uLFR HT DR - CODMn-04-E (20160411)